


A GUIDE TO THE
**Use and Calibration
of Detector Array
Equipment**

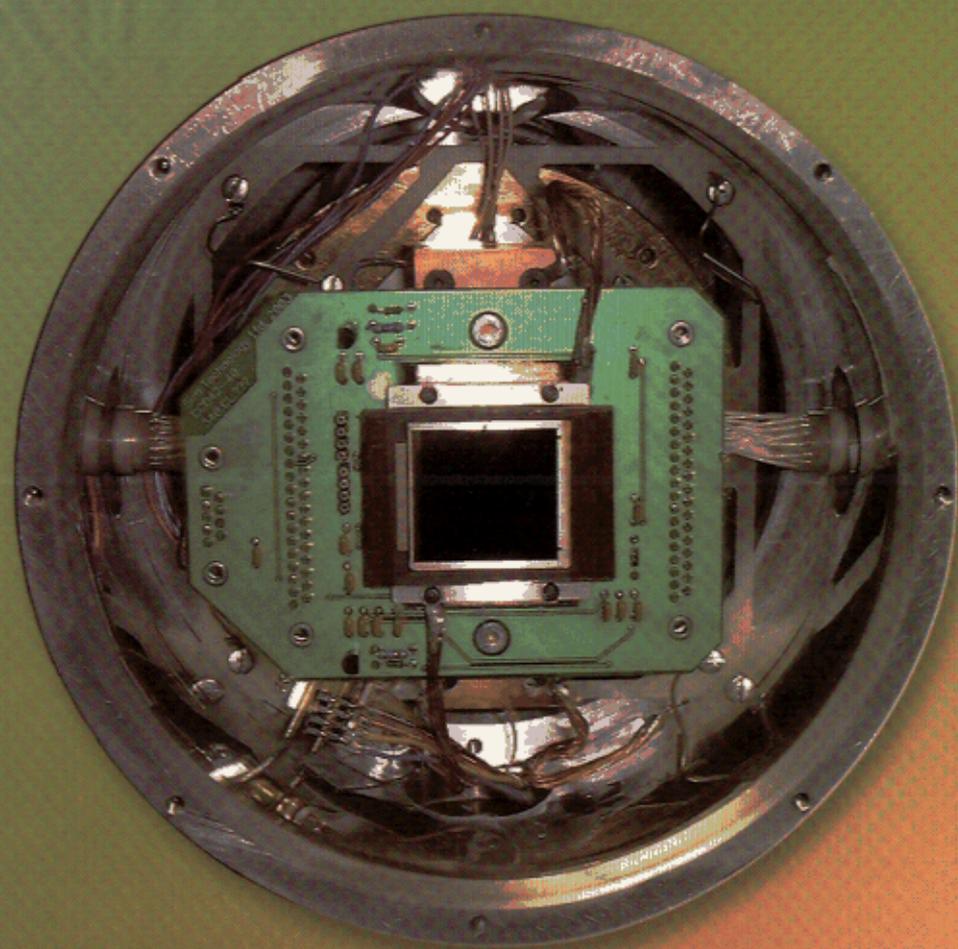

Gordon R. Hopkinson • Teresa M. Goodman • Stuart R. Prince

CONTENTS

<i>Introduction</i>	<i>ix</i>
Chapter 1 Detector Arrays	1
1.1 Types of Detector Arrays	1
1.1.1 Types of Silicon Detector Arrays	3
1.1.2 Color Imaging	10
1.1.3 Intensified CCDs	12
1.1.4 Specialized CCD Readout Modes	13
1.1.5 Resetting of Output Amplifiers and Pixels	19
1.1.6 Readout of IR arrays	21
1.2 Key Parameters and Their Measurement	23
1.2.1 Units	24
1.2.2 Electrical Test Methods	25
1.2.3 Measurements on Dark Images	25
1.2.4 Offset Level	27
1.2.5 Average Dark Signal	27
1.2.6 Dark Signal Nonuniformity (DSNU)	28
1.2.7 Fixed Pattern Noise (FPN)	29
1.2.8 Photo-Response Nonuniformity (PRNU)	30
1.2.9 Charge-to-Voltage Conversion Factor (CVF) and Conversion Gain	32
1.2.10 Temporal Noise	36
1.2.11 Linearity	38
1.2.12 Full Well Capacity (Saturation)	39
1.2.13 Charge Transfer Efficiency (CTE) of a CCD	40
1.2.14 Modulation Transfer Function (MTF)	42
1.2.15 Responsivity (and Spectral Responsivity)	45
1.2.16 Quantum Efficiency (QE)	47
1.2.17 Lag	47
1.2.18 Crosstalk	48
1.2.19 Geometrical Measurements	49
1.3 Photometric versus Radiometric Units	49
1.4 Output Signal Calculations	51
References	52

Chapter 2 Detector Array Equipment and Requirements for Calibration	57
2.1 Imaging Applications	58
2.1.1 Machine Vision	58
2.1.2 Photometric/Radiometric Imaging	58
2.1.3 Color Measurement	59
2.1.4 Earth Remote Sensing	60
2.1.5 Fluorescence Microscopy	60
2.1.6 Photogrammetry, Profilometry, and Noncontact Metrology	61
2.1.7 Thermal Imaging	61
2.2 Spectrometry Applications	61
2.2.1 General Spectroscopy	63
2.2.2 Absorbance and Reflectance Spectrometry	63
2.2.3 Emission Spectrometry	64
2.2.4 Vibrational Spectrometry	65
2.2.5 Multichannel Raman Spectroscopy	65
2.2.6 Imaging Spectroscopy	66
2.3 Other Applications	67
References	68
Chapter 3 Influence of Array Parameters on Instrument Calibration	71
3.1 Key Array Parameters	71
3.1.1 Quantum Efficiency (QE)	73
3.1.2 On-Chip Amplifier Response	76
3.1.3 Off-Chip Electronics Gain	76
3.1.4 Response Nonuniformity (Interpixel)	77
3.1.5 Response Nonuniformity (Intrapixel)	85
3.1.6 Stray Light	89
3.1.7 Dark Signal and Dark Signal Nonuniformity	89
3.1.8 Nonlinearity	93
3.1.9 Full Well Capacity	94
3.1.10 Noise	95
3.1.11 Crosstalk Between Pixels	96
3.1.12 Lag	97
3.1.13 Resolution and MTF	99
3.1.14 Aliasing	100
3.1.15 Cosmic Ray Effects	101
3.1.16 Smear	102
3.1.17 Geometrical Stability	103
3.1.18 Image Anomalies	104
3.1.19 Electrical Parameters	106
3.2 Intensified Arrays	106
3.3 Conclusions	107
References	108

Chapter 4 Calibration Techniques for Instruments	113
4.1 Imaging Instruments	113
4.1.1 Silicon-based Array Systems	113
4.1.2 Thermal Imagers	116
4.2 Instruments for Spectrometry	121
4.2.1 Definitions	123
4.2.2 Wavelength Calibration	123
4.2.3 Responsivity	136
4.2.4 Stray Light	140
4.2.5 Linearity	148
4.2.6 Dark Reading and External Stray Light	159
4.3 Multichannel Raman and Emission Spectrometers	161
4.3.1 Wavelength Calibration	161
4.3.2 Intensity Calibration	163
4.4 Imaging Spectrometers	164
4.4.1 MTF Testing	165
4.4.2 Wavelength Accuracy	165
4.4.3 Smile	165
4.4.4 Frown	166
References	166
Chapter 5 Calibration Equipment	173
5.1 Sources	173
5.1.1 Continuum Sources	173
5.1.2 Line Sources	181
5.1.3 Other Sources	182
5.1.4 Suppliers of Light Sources	183
5.2 Filters	184
5.2.1 Neutral Density Filters	184
5.2.2 Other Filters	184
5.2.3 Suppliers of Filters	185
5.3 Ceramic Tiles	185
5.4 Grids and Resolution Charts	186
5.5 Cells for Absorption Spectroscopy	186
5.6 Contact Details	186
References	187
Chapter 6 Comparison of International Standards	189
Appendix A Reference Guide	191
A.1 Calibration services and contacts	191
A.1.1 Accreditation	191
A.1.2 Calibration	191

A.2 Bibliography—including general articles, books, and useful websites	192
A.2.1 General	192
A.2.2 Arrays	192
A.2.3 Instrumentation	193
A.2.4 Calibration	194
A.3 List of Abbreviations	196
Appendix B Glossary of Terms	199
Appendix C Quick Guide to Recommended Calibration Procedures	213
C.1 Spectrometers	213
C.1.1 Wavelength Calibration	213
C.1.2 Responsivity	214
C.1.3 Stray Light	214
C.1.4 Linearity	215
C.1.5 Dark Reading and External Stray Light	215
C.2 Imagers	216
Index	217